

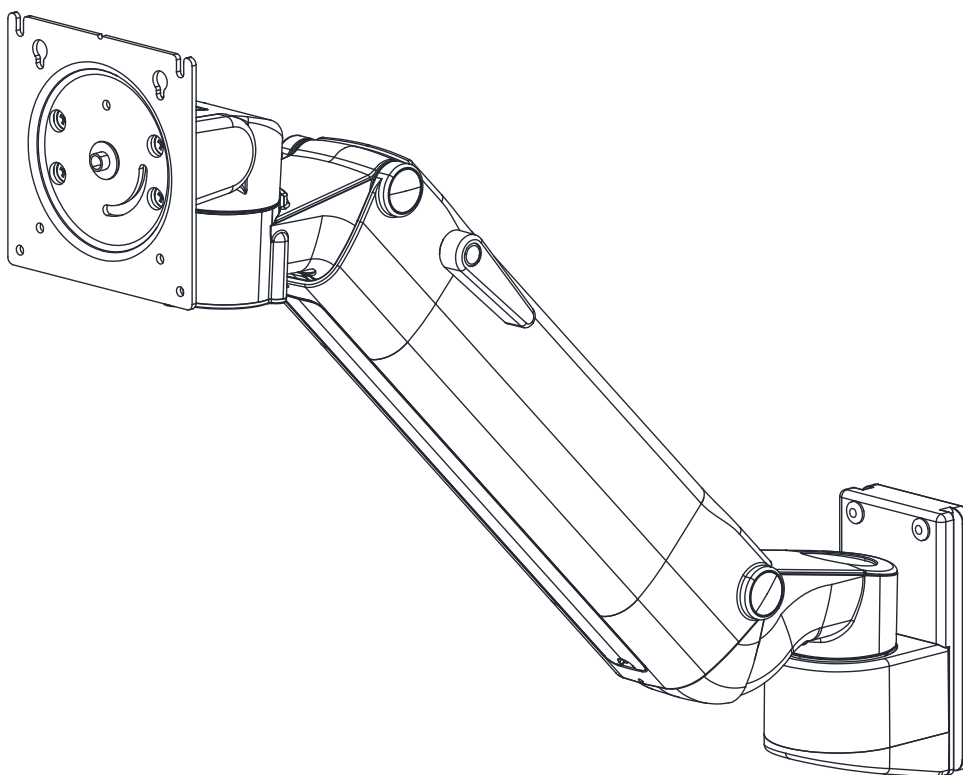







Installation Guide

MHA Variable Height Patient Monitor Arm
DG-013-022W,DG-013-032W



 1X 	1X  3MM	1X  4MM	1X  screwdriver	8X  M4x10,M4x14
--	--	--	---	--

Akiteck International Pte Ltd

ADD: 280 WOODLANDS INDUSTRIAL PARK E5, #06-44, HARVEST
@ WOODLANDS, Singapore 757322

Singapore Line: +65 9671 2188


China Line: +86 134 2488 9887

E-mail: marcus@akiteck.com.sg




Installation Steps


1

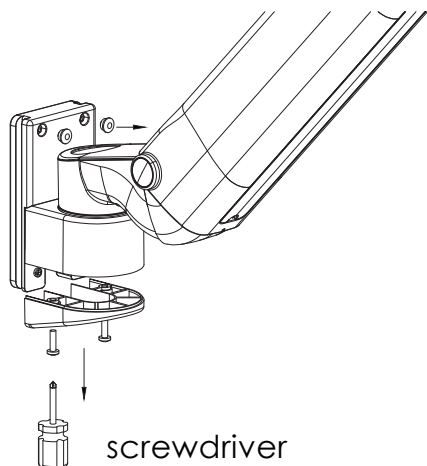


2

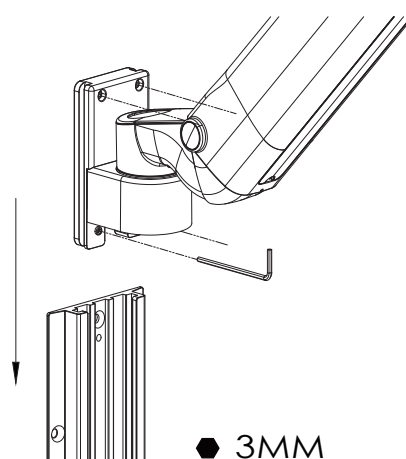


3

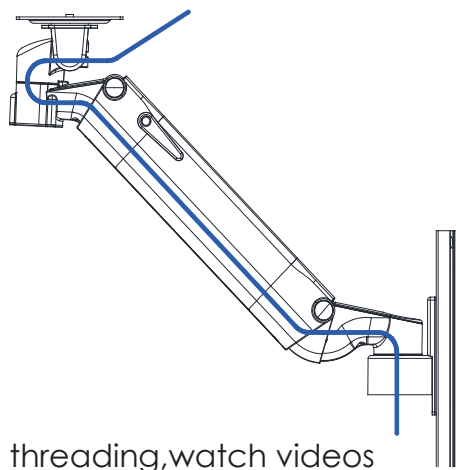

4

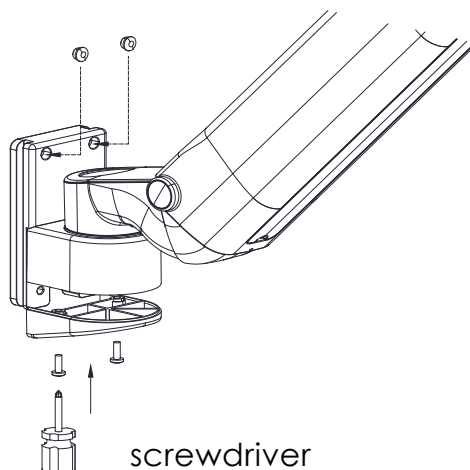

5

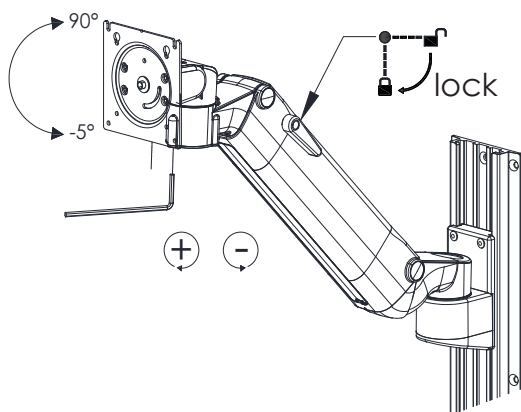

Akitek International Pte Ltd

ADD: 280 WOODLANDS INDUSTRIAL PARK E5, #06-44, HARVEST
@ WOODLANDS, Singapore 757322

Singapore Line: +65 9671 2188

China Line: +86 134 2488 9887

E-mail: marcus@akitek.com.sg